



200201696001


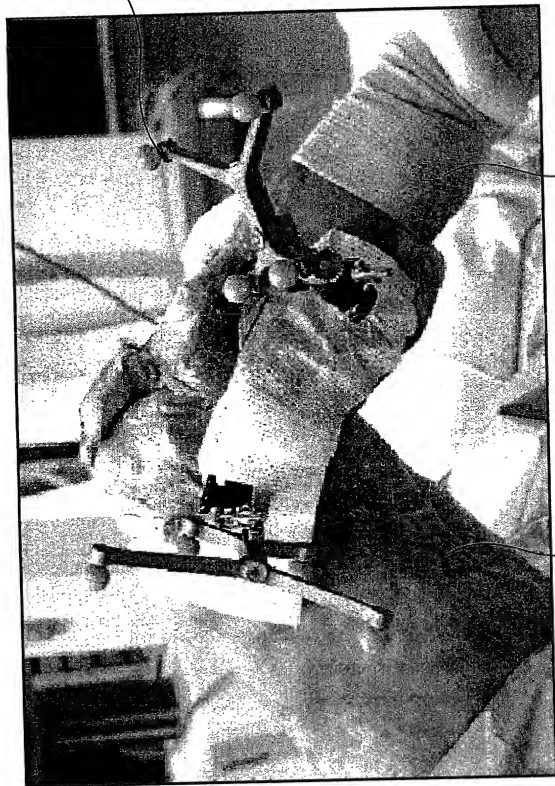


Fig. 2

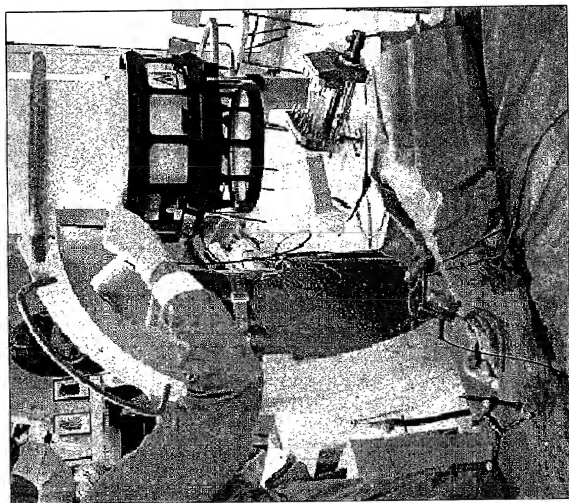

14

Fig. 3

NOTES

CSI Medical Systems - Minneapolis  
8811

Not Saved

PNR 14

Edge 60  
Zoom 1.0  
Edge 400  
Cost 400

24

Free space 4000  
Max seq 1000

Fig. 4

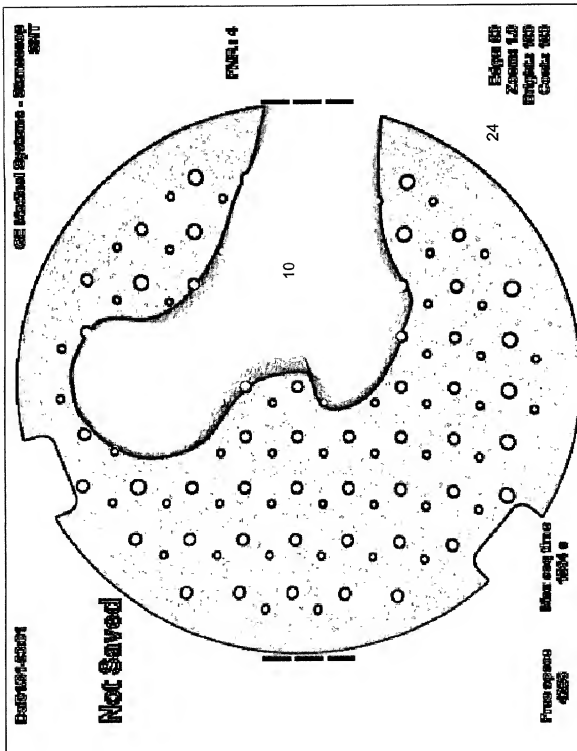


Fig. 5

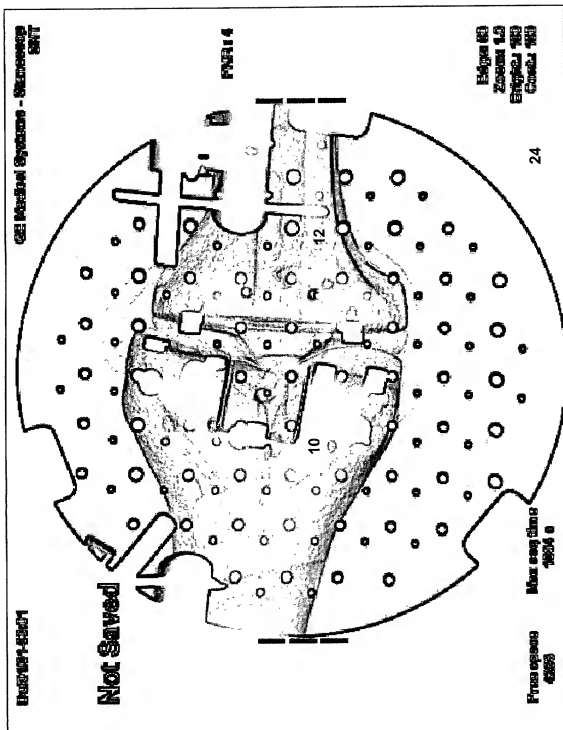


Fig. 6

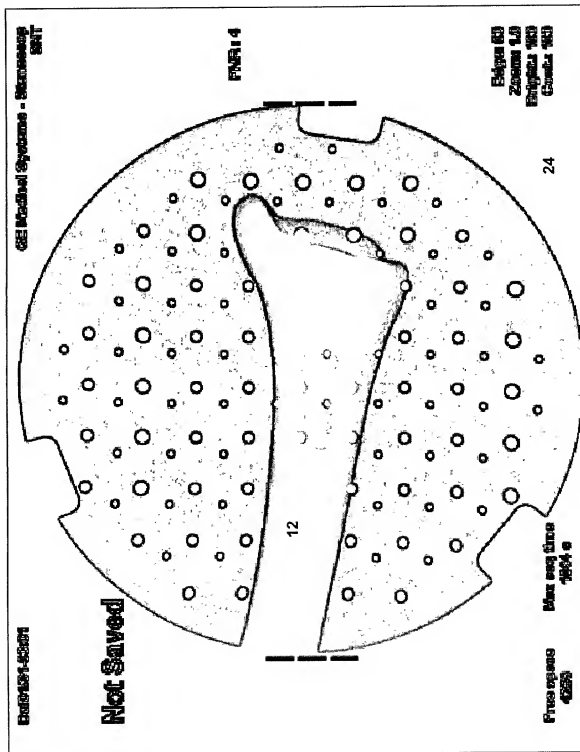


Fig. 7

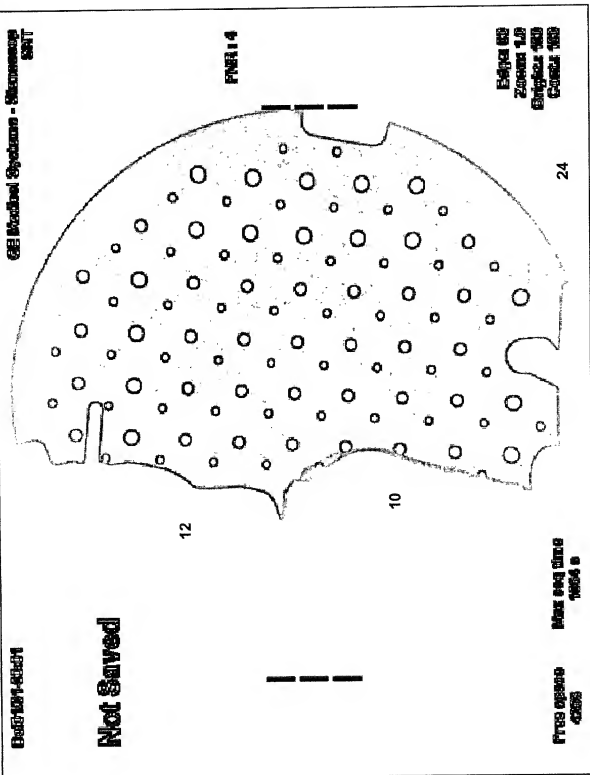


Fig. 8



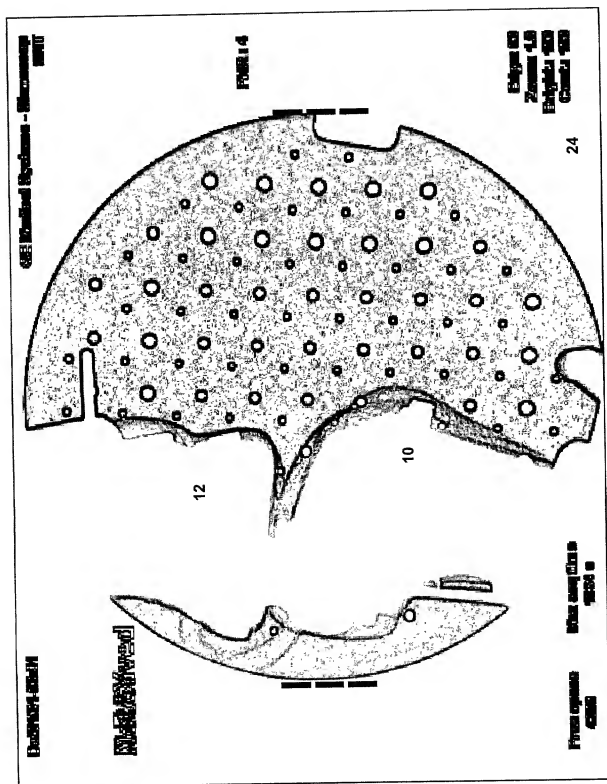


Fig. 9

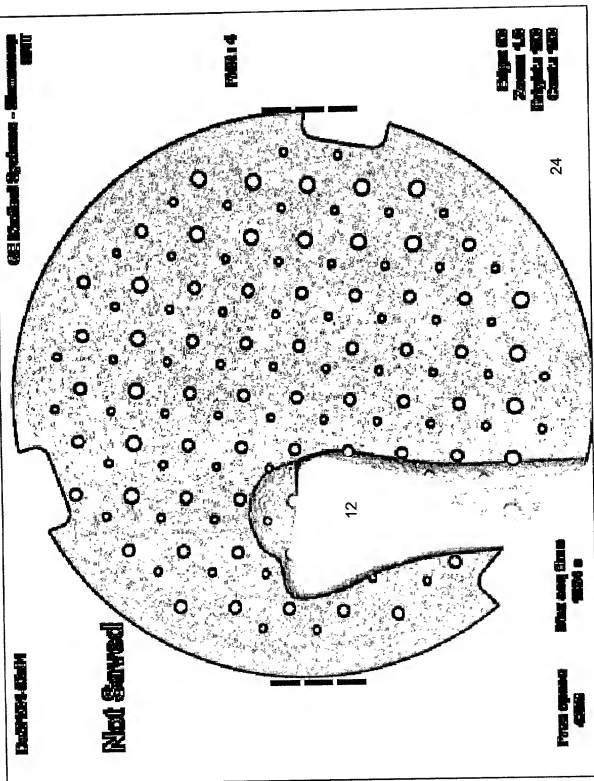


Fig. 10

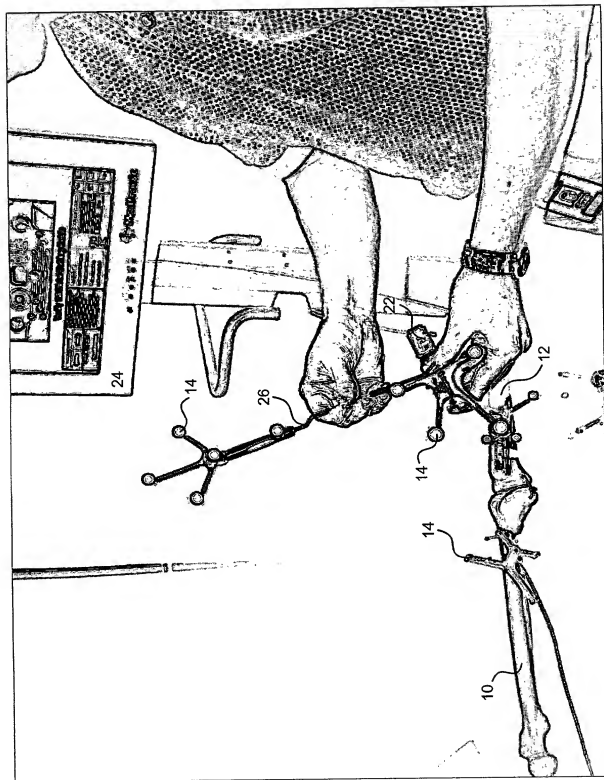


Fig. 11

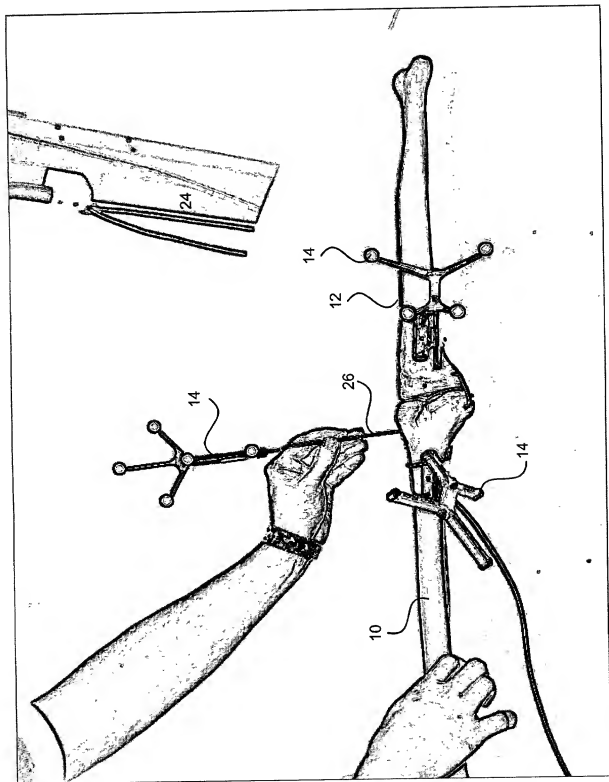


Fig. 12

# Determine Femoral Mechanical Axis

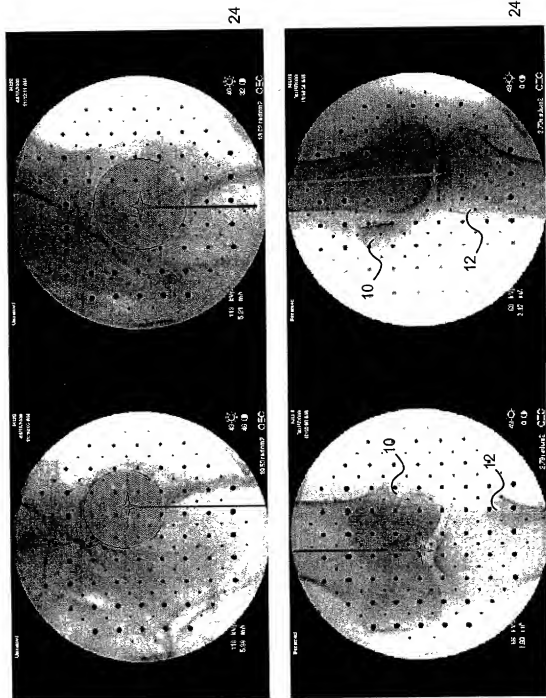


Fig. 13

# Determine Epicondylar Axis

24

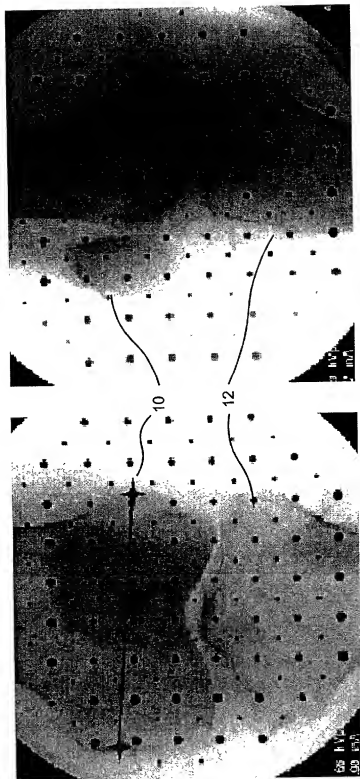


Fig. 14

# Determine Anterior-Posterior Axis

24

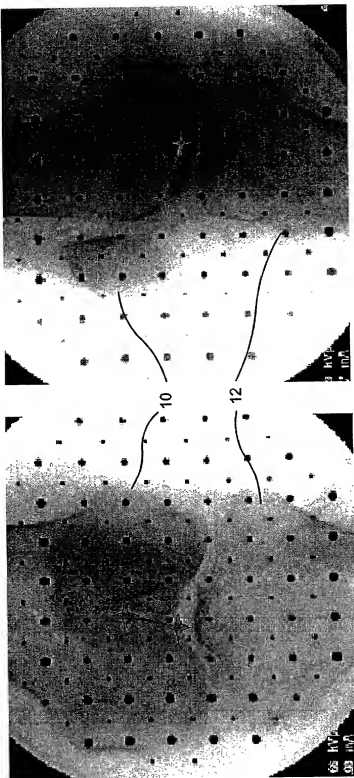


Fig. 15



Fig. 16



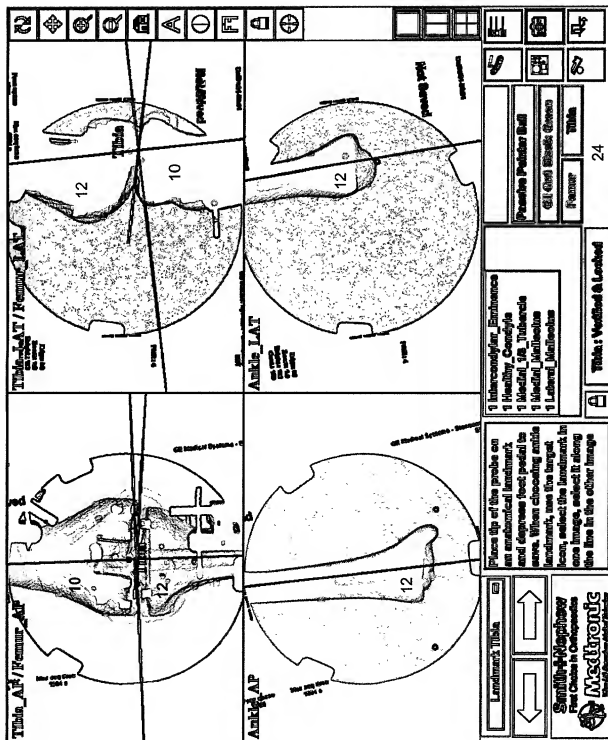


Fig. 17

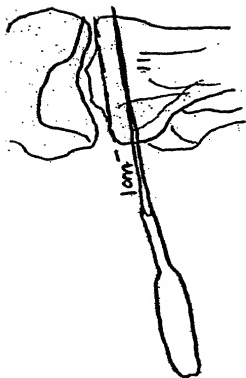


Fig. 18





Fig. 19

202501160001

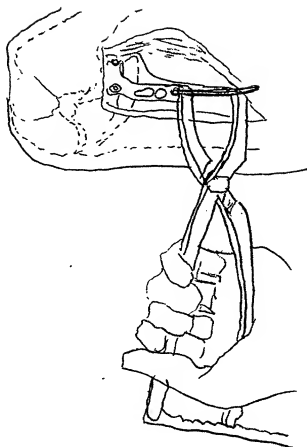


Fig. 20



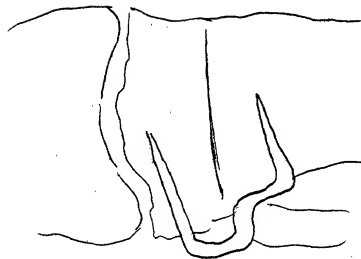


Fig. 22